

UNITED STATES PATENT AND TRADEMARK OFFICE

BEFORE THE PATENT TRIAL AND APPEAL BOARD

CORPAK MEDSYSTEMS, INC. and HALYARD HEALTH, INC.,
Petitioners,

v.

KIRN MEDICAL DESIGN, L.L.C. and APPLIED MEDICAL
TECHNOLOGY, INC.,
Patent Owner.¹

Case IPR2017-00646
Patent 6,631,715 B2

Before PATRICK R. SCANLON, JAMES A. WORTH, and
JAMES J. MAYBERRY, *Administrative Patent Judges*.

SCANLON, *Administrative Patent Judge*.

DECISION

Denying Institution of *Inter Partes* Review
35 U.S.C. § 314 and 37 C.F.R. § 42.108

¹ The Mandatory Notices provided by Applied Medical Technology, Inc. (“AMT”) identify Kirn Medical Design, L.L.C. (“Kirn”) as the owner of the ’715 patent and AMT as the exclusive licensee of the ’715 patent, and both entities as real parties-in-interest in this proceeding. Paper 5, 2. In addition, AMT has provided a statement from Kirn confirming that AMT is the exclusive licensee of the ’715 patent and consenting to AMT defending the ’715 patent in this proceeding. *Id.* at 5.

I. INTRODUCTION

Corpak Medsystems, Inc. and Halyard Health, Inc. (“Petitioners”) filed a Petition (Paper 1, “Pet.”) requesting an *inter partes* review of claim 18 of U.S. Patent No. 6,631,715 B2 (Ex. 1001, “the ’715 patent”). Applied Medical Technology, Inc. (“AMT”), the exclusive licensee of the ’715 patent, filed a Preliminary Response (Paper 7, “Prelim. Resp.”).

We have jurisdiction under 35 U.S.C. § 314, which provides that *inter partes* review may not be instituted unless “the information presented in the petition . . . and any [preliminary] response . . . shows that there is a reasonable likelihood that the petitioner would prevail with respect to at least 1 of the claims challenged in the petition.” 35 U.S.C. § 314(a).

Upon consideration of the arguments and evidence presented by Petitioners and AMT, we are not persuaded that Petitioners have demonstrated, under 35 U.S.C. § 314(a), a reasonable likelihood that it would prevail in showing the unpatentability of claim 18. Accordingly, we do not institute an *inter partes* review.

II. BACKGROUND

A. *Related Matters*

The parties indicate that the ’715 patent is at issue in the following related case: *Applied Med. Tech., Inc. v. Corpak Medsystems, Inc.*, No. 1:16-cv-02190 (N.D. Ohio). Pet. 6; Paper 5, 2.

B. *The ’715 patent*

The ’715 patent, titled “Magnetic Nasal Tube Bridle System and Related Method,” issued on October 14, 2003. Ex. 1001, (45), (54). The ’715 patent “relates generally to systems for placing and securing a nasal tube; and more particularly to such a system which utilizes magnets in the

placement of a bridle used in combination with a receiver to secure the nasal tube.” *Id.* at 1:8–12.

In one embodiment, flexible member 10 is used to secure a nasal tube in a patient. *Id.* at 4:16–17. Flexible member 10 is a soft, flexible tube having magnet 13 attached to end portion 12. *Id.* at 4:23–26, Fig. 1. In addition, flexible member 10 is long enough to be able to loop around the patient’s nasal septum so that each end of flexible member 10 extends through a respective nare or nostril of the patient. *Id.* at 4:17–21, Fig. 7d.

Magnetic probe 20 is inserted into a nare to attract magnet 13 and retrieve end portion 12 of flexible member 10. *Id.* at 4:54–56. Magnetic probe 20 is a rigid or semi-rigid cylinder having magnet 21 attached to first end portion 22. *Id.* at 4:57–61, Fig. 3. The polarity of magnet 21 is opposite the polarity of magnet 13 so that the two magnets attract. *Id.* at 5:1–4.

A method of placing and securing a nasal tube in a patient includes inserting the tube into a nare of the patient’s nose, inserting end portion 12 of flexible member 10 into a first nare, inserting magnetic probe 20 into a second nare to attract end portion 12, and removing magnetic probe 20 so as to retrieve end portion 12 through the second nare. *Id.* at 6:19–28, Figs. 7a–7c. Specifically, end portion 12 (and thus magnet 13) is inserted into the first nare beyond the posterior border of nasal septum N through the choanal aperture. *Id.* at 6:34–40, Fig. 7b. When magnetic probe 20 is inserted similarly into the second nare, it attracts and connects with magnet 13 of flexible member 10, thus allowing end portion 12 to be retrieved through the second nare. *Id.* at 6:47–52. That is, magnetic probe 20 is withdrawn from the second nare, thereby pulling magnetically coupled flexible member 10 “into the first nare and out through the second nare.” *Id.* at 6:60–64, Fig. 7c.

This process results in flexible member 10 being looped posteriorly around nasal septum N (*id.* at 6:64–66), as shown in Figure 7d of the '715 patent, which is reproduced below.


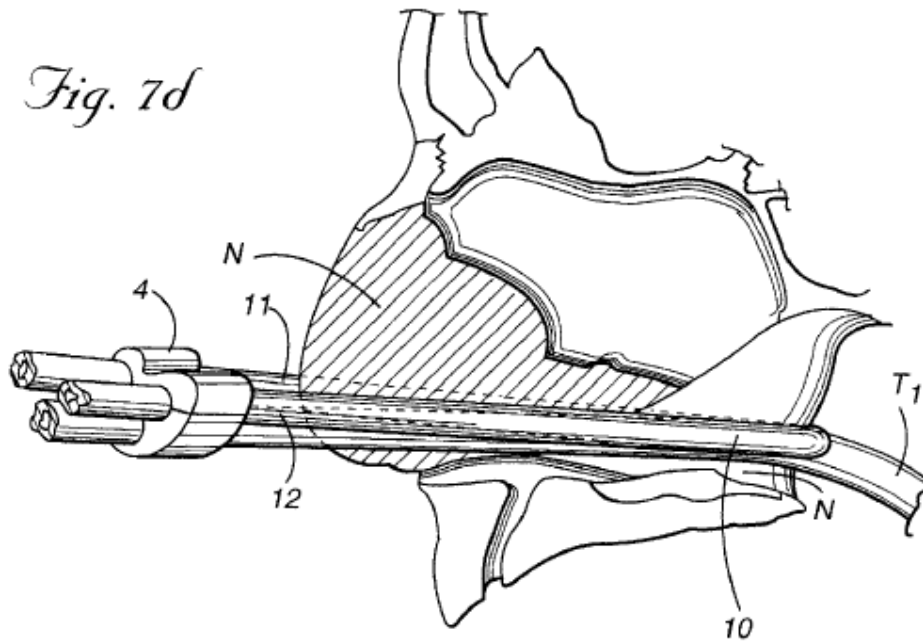


Figure 7d depicts flexible member 10 looped posteriorly around nasal septum N and magnetic probe 20 separated from end portion 12. *Id.* at 6:64–7:2. Receiver 24² is secured to end portions 11, 12 of flexible member 10 and to nasal tube T₁, which is inserted into one of the patient's nares. *Id.* at 7:3–13, Fig. 7d.

Figures 4 and 5 of the '715 patent are reproduced below.

² The receiver is misidentified in Figure 7d with reference numeral 4.

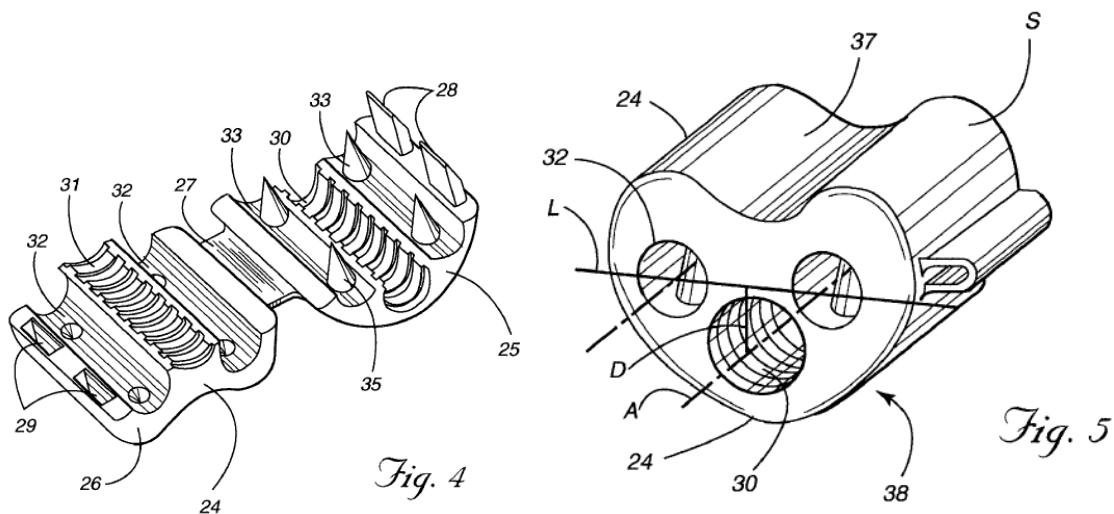

Figures 4 and 5 depict receiver 24 for securing nasal tube T_1 and end portions 11, 12 of flexible member 10, with Figure 4 showing receiver 24 in an open position for receiving the nasal tube and the flexible member ends. *Id.* at 3:56–58, 5:8–10. Receiver 24 comprises two members 25, 26 pivotally connected by living hinge 27. *Id.* at 5:11–15, Fig. 4. Snap-type locking hooks 28 extend from member 25, and mating holes 29 are formed in member 26 for firmly securing the members together over nasal tube T_1 and end portions 11, 12. *Id.* at 5:15–19, Fig. 4.

Receiver 24 includes first channel 30 formed in member 25 for receiving nasal tube T_1 . *Id.* at 5:23–24, Figs. 4, 5. Mating channel 31 may be formed in member 26, such that channels 30, 31 form a hole through receiver 24 for firmly grasping nasal tube T_1 . *Id.* at 5:32–35, Figs. 4, 5. Receiver 24 further includes two sets of channels 32, 33 for receiving and securing end portions 11, 12 of flexible member 10. *Id.* at 5:37–43, Figs. 4, 5.

Explore Litigation Insights

Docket Alarm provides insights to develop a more informed litigation strategy and the peace of mind of knowing you're on top of things.

Real-Time Litigation Alerts



Keep your litigation team up-to-date with **real-time alerts** and advanced team management tools built for the enterprise, all while greatly reducing PACER spend.

Our comprehensive service means we can handle Federal, State, and Administrative courts across the country.

Advanced Docket Research



With over 230 million records, Docket Alarm's cloud-native docket research platform finds what other services can't. Coverage includes Federal, State, plus PTAB, TTAB, ITC and NLRB decisions, all in one place.

Identify arguments that have been successful in the past with full text, pinpoint searching. Link to case law cited within any court document via Fastcase.

Analytics At Your Fingertips



Learn what happened the last time a particular judge, opposing counsel or company faced cases similar to yours.

Advanced out-of-the-box PTAB and TTAB analytics are always at your fingertips.

API

Docket Alarm offers a powerful API (application programming interface) to developers that want to integrate case filings into their apps.

LAW FIRMS

Build custom dashboards for your attorneys and clients with live data direct from the court.

Automate many repetitive legal tasks like conflict checks, document management, and marketing.

FINANCIAL INSTITUTIONS

Litigation and bankruptcy checks for companies and debtors.

E-DISCOVERY AND LEGAL VENDORS

Sync your system to PACER to automate legal marketing.