

UNITED STATES PATENT AND TRADEMARK OFFICE

BEFORE THE PATENT TRIAL AND APPEAL BOARD

SOTERA WIRELESS, INC.,
Petitioner,

v.

MASIMO CORPORATION,
Patent Owner.

IPR2020-01078
Patent RE47,218 E

Before GEORGE R. HOSKINS, JENNIFER MEYER CHAGNON, and
AMANDA F. WIEKER, *Administrative Patent Judges*.

HOSKINS, *Administrative Patent Judge*.

DECISION
Granting Institution of *Inter Partes* Review
35 U.S.C. § 314

I. INTRODUCTION

Sotera Wireless, Inc. (“Petitioner”) has filed a Petition (Paper 1, “Pet.”) pursuant to 35 U.S.C. §§ 311–319 to institute an *inter partes* review of claims 1–10 and 12–18 of U.S. Patent No. RE47,218 E (“the ’218 patent”).

Masimo Corporation (“Patent Owner”) has filed a Preliminary Response (Paper 6, “Prelim. Resp.”) to the Petition.

We authorized additional briefing to address Patent Owner’s argument that we should deny institution under 35 U.S.C. § 314(a) and *Apple Inc. v. Fintiv, Inc.*, IPR2020-00019, Paper 11 (PTAB Mar. 20, 2020) (precedential) (“*Fintiv* Order”). See Paper 7. Accordingly, Petitioner filed a Reply (Paper 10, “Prelim. Reply”) to the Preliminary Response, and Patent Owner filed a Sur-reply (Paper 11, “Prelim. Sur-reply”) to the Reply.

Institution of review requires Petitioner to demonstrate a reasonable likelihood of prevailing with respect to at least one challenged claim. 35 U.S.C. § 314(a). Applying that standard on behalf of the Director (37 C.F.R. § 42.4(a)), we institute an *inter partes* review to determine whether Petitioner demonstrates by a preponderance of the evidence that claims 1–10 and 12–18 are unpatentable.

II. BACKGROUND

A. Real Parties-in-Interest and Related Proceedings

Sotera Wireless, Inc. and Hon Hai Precision Industry Co., Ltd. are the real parties-in-interest for Petitioner, and Masimo Corporation is the real party-in-interest for Patent Owner. Pet. 1; Paper 5, 1. Also, *Masimo Corp. v. Sotera Wireless, Inc. and Hon Hai Precision Industry Co. Ltd.*, Civil

Action No. 3:19-cv-01100-BAS-NLS (S.D. Cal.) (“the District Court Litigation”) is a related judicial matter. Pet. 2; Paper 5, 1.

B. The '218 Patent

The '218 patent concerns a system for monitoring a patient's blood oxygen saturation (SpO_2), and generating an alarm if the saturation falls too low. *See* Ex. 1001, Abstract, 1:34–39, 2:54–58. The system includes an optical sensor attached to the patient's finger, to emit light into the fingertip tissue and detect light that is attenuated by blood flow within the fingertip, to provide a numerical readout of oxygen saturation. *See id.* at 1:39–55.

Figure 1 of the '218 patent is reproduced here:

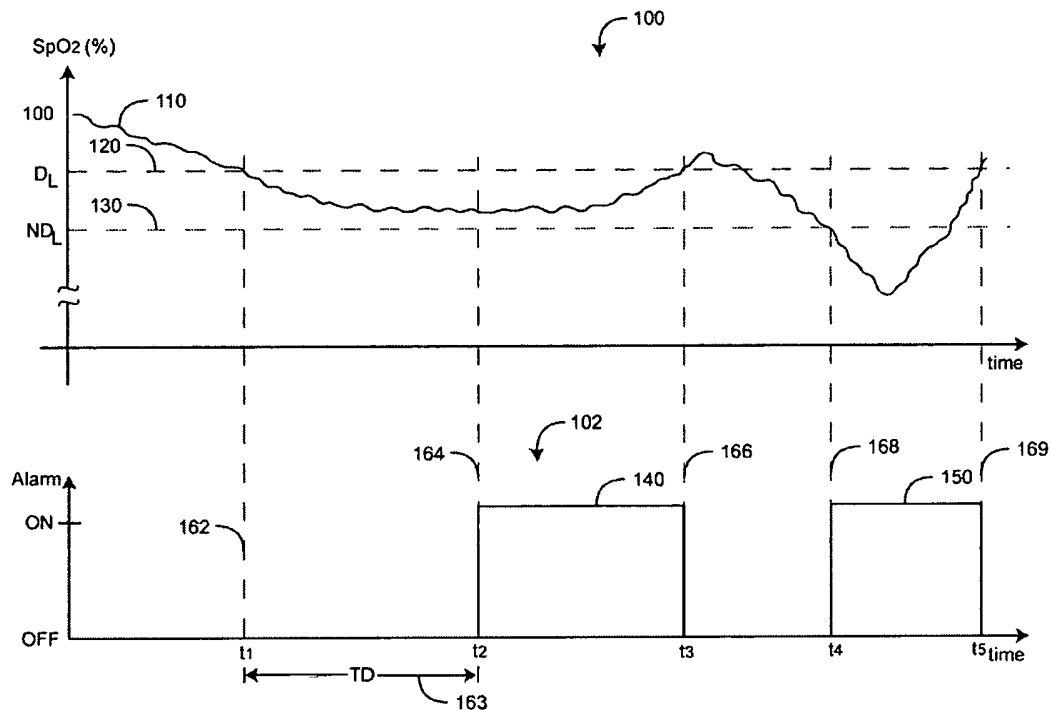


Figure 1 of the '218 Patent.

Figure 1 illustrates a previously known oxygen saturation measurement system having two “fixed-threshold alarm” schemes, at “delay” alarm threshold D_L and at “no delay” alarm threshold ND_L . *Id.* at 2:54–59

(emphasis added). If the patient's measured oxygen saturation 110 falls and stays below delay threshold D_L for a time period greater than time delay TD , as shown in Figure 1 from time t_1 to time t_2 , then delayed alarm 140 is triggered. *Id.* at 2:59–3:1. If the patient's measured oxygen saturation 110 falls below no delay threshold ND_L , as shown in Figure 1 at time t_4 , then immediate alarm 150 is triggered without delay. *Id.* at 2:61–62, 3:2–4.

According to the '218 patent, the fixed nature of delay alarm threshold D_L undesirably leads to “a baseline drift problem,” which can generate a “nuisance” or “false” alarm. *Id.* at 2:54–56, 3:24–46 (describing Fig. 3). The '218 patent therefore proposes “an adaptive alarm system,” which adjusts the delay alarm threshold downwards when an oxygen saturation baseline is established at lower values. *Id.* at 3:59–62. In this way, the inventive “alarm threshold . . . adapts to baseline drift in [oxygen saturation] and reduce[s] false alarms without a corresponding increase in missed true alarms.” *Id.* at 4:4–8.

This is illustrated in Figure 6 of the '218 patent, reproduced here:

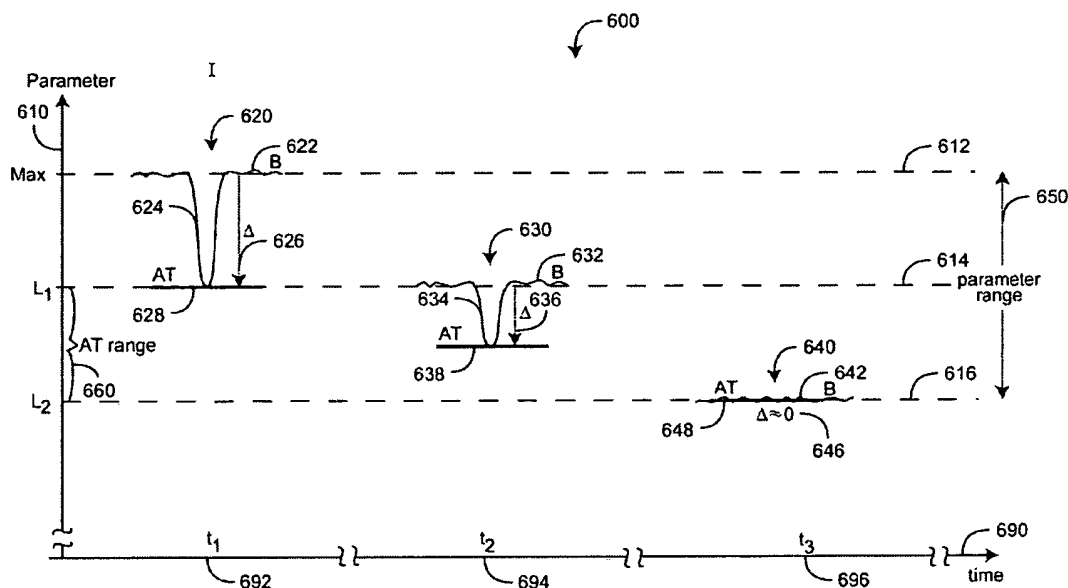


Figure 6 of the '218 Patent.

Figure 6 graphs a measured physiological parameter such as oxygen saturation (the vertical axis) over time (the horizontal axis), as generated by an alarm system having a lower limit adaptive alarm threshold AT. *Id.* at 5:34–36, 7:40–47. An adaptive alarm threshold AT is applied whenever the measured oxygen saturation falls within range 650, extending from lower limit L_2 up to maximum value Max, such as illustrated at segments 620, 630, and 640. *Id.* at 6:15–30, 7:9–67, Fig. 5B (horizontal axis values extend from L_2 to Max). The adaptive thresholds AT are constrained to lie within range 660, extending from lower limit L_2 up to limit L_1 . *Id.* at 6:15–30, 7:9–67, Fig. 5A (adaptive threshold AT line 442 is constrained between limits L_1 and L_2 along vertical axis).

In a preferred embodiment, lower limit L_2 is equal to the no delay alarm threshold ND_L of the prior art system shown in Figure 1, and limit L_1 is equal to the delay alarm threshold D_L of the prior art system. *Id.* at 5:66–6:4, 6:20–34. However, the fixed threshold the prior art implements at limit L_1 is replaced by adaptive thresholds AT. *Id.* at 6:22–34. Each individual threshold AT, during a given time period such as t_1 , t_2 , or t_3 , may advantageously be implemented as a time delay alarm, as the prior art system does with its fixed delay alarm threshold D_L . *Id.* at 6:38–43.

The system determines a baseline B of the patient's oxygen saturation during different time periods such as t_1 , t_2 , and t_3 . *Id.* at 6:11–15, 6:44–7:8. For each different baseline B, the system applies a different adaptive alarm threshold AT. *Id.* at 6:15–19, Fig. 6. Specifically, the system calculates delta Δ as a function of the varying baseline B and the pre-set limits L_1 and L_2 and maximum value Max. *Id.* at 6:15–34 (describing Fig. 4A), 7:9–39 (describing Fig. 5B). Then, the adaptive alarm threshold is set at

Explore Litigation Insights

Docket Alarm provides insights to develop a more informed litigation strategy and the peace of mind of knowing you're on top of things.

Real-Time Litigation Alerts



Keep your litigation team up-to-date with **real-time alerts** and advanced team management tools built for the enterprise, all while greatly reducing PACER spend.

Our comprehensive service means we can handle Federal, State, and Administrative courts across the country.

Advanced Docket Research



With over 230 million records, Docket Alarm's cloud-native docket research platform finds what other services can't. Coverage includes Federal, State, plus PTAB, TTAB, ITC and NLRB decisions, all in one place.

Identify arguments that have been successful in the past with full text, pinpoint searching. Link to case law cited within any court document via Fastcase.

Analytics At Your Fingertips



Learn what happened the last time a particular judge, opposing counsel or company faced cases similar to yours.

Advanced out-of-the-box PTAB and TTAB analytics are always at your fingertips.

API

Docket Alarm offers a powerful API (application programming interface) to developers that want to integrate case filings into their apps.

LAW FIRMS

Build custom dashboards for your attorneys and clients with live data direct from the court.

Automate many repetitive legal tasks like conflict checks, document management, and marketing.

FINANCIAL INSTITUTIONS

Litigation and bankruptcy checks for companies and debtors.

E-DISCOVERY AND LEGAL VENDORS

Sync your system to PACER to automate legal marketing.